


Equipment Technical Bulletin

Rerating of Alarm Output Relay on Summit



Beta Technology documentation rates the alarm output relay at 1A 125 VAC (or VDC). This rating is incorrect for the Summit as currently designed. The relay should be rated 1A 24V. If you are currently using the relay with voltage greater than 24V please disconnect it and contact Beta Technology Technical Support for installation alternatives.

A design change is underway to enable usage of the relay with line power. A subsequent ETB will announce when that design revision is available.

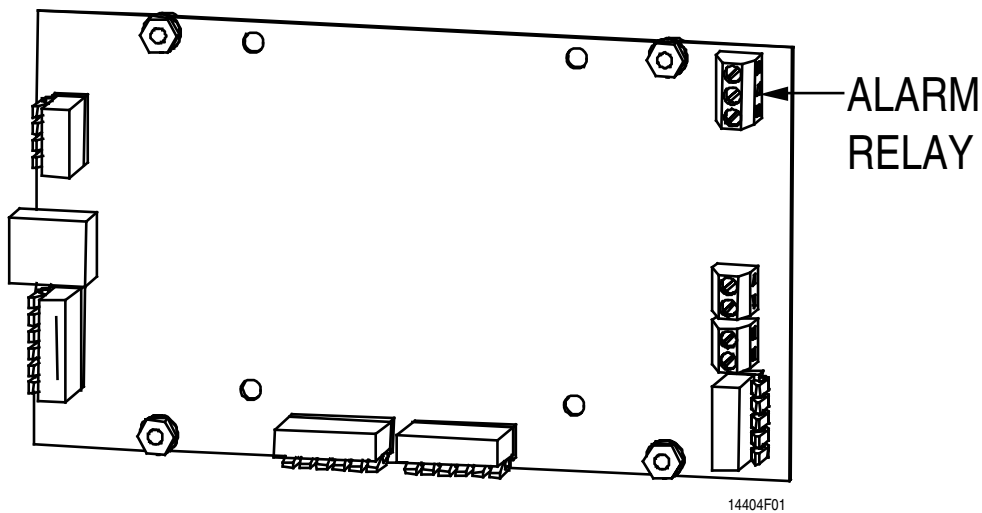

Beta Technology, Inc
 2841 Mission Street
 Santa Cruz • CA
 U.S.A. • 95060

TEL • 831 • 426 • 0882
 TEL • 800 • 858 • 2382
 FAX • 831 • 423 • 4573
 FAX • 800 • 221 • 8416
 TEL • 800 • 215 • 6415 | Tech Support
 sales@beta-technology.com

Customer Service

Beta Technology, Inc
 4 Firway, Dallow Road
 Luton LU1 1TR
 United Kingdom

Freephone • 0800 • 052 • 4726
 Tel • +44(0) • 1582 • 528600
 Fax • +44(0) • 1582 • 528111
 Freephone • 0800 • 052 • 4726 | Tech Service
 VAT REG.NO.BG.354 - 09975 - 44
 europe.sales@beta-technology.com

Customer Service

Online Ordering: <http://www.beta-technology.com>